

Crypto/Giardia Duo-Strip


Rapid diagnostic test for *in vitro* detection of *Cryptosporidium* & *Giardia* in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')
- 2x-sided sticks



www.corisbio.com

Crypto/Giardia Duo-Strip

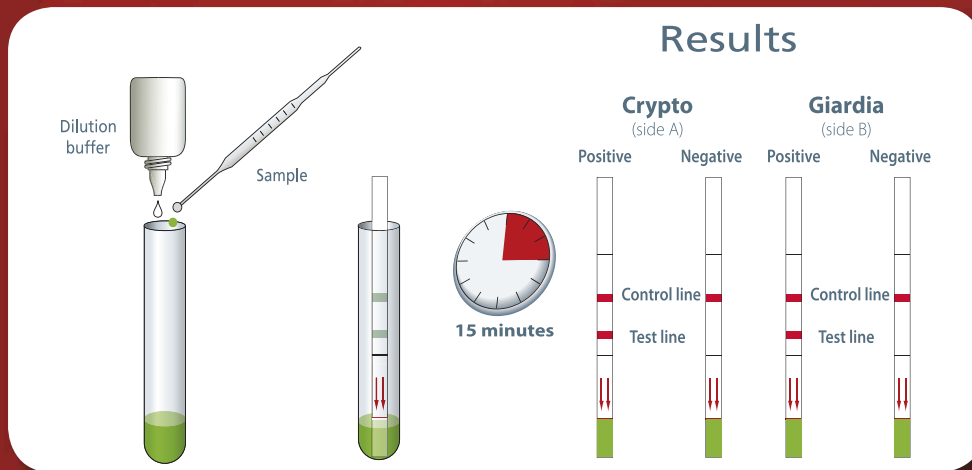

Performance compared to

	ICT competitor (n=100)	Microscopy (n=382)
	Crypto	Giardia
Specificity	100% (53/53)	97.8% (309/316)
Sensitivity	95.7% (45/47)	96.3% (77/80)
PPV	100% (45/45)	91.7% (77/84)
NPV	96.4% (53/55)	99% (309/312)
Accuracy	98% (98/100)	97.5% (386/396)

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
Crypto/Giardia Duo-Strip	25 tests, buffer	4°C to 30°C	C-1018
Crypto/Giardia Uni-Strip	10 individual strips, buffer, sample taking material (test tubes, loops, tube holder)	4°C to 30°C	C-1518

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, Mefloquine, Proguanil, *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

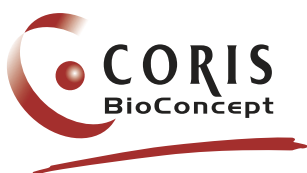

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-18/02
January 2012