

Influ-A Respi-Strip


Rapid diagnostic test for *in vitro* detection of Influenza A Virus in swabs, washings or aspirates of nasopharyngeal secretions

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')



www.corisbio.com

Influ-A Respi-Strip

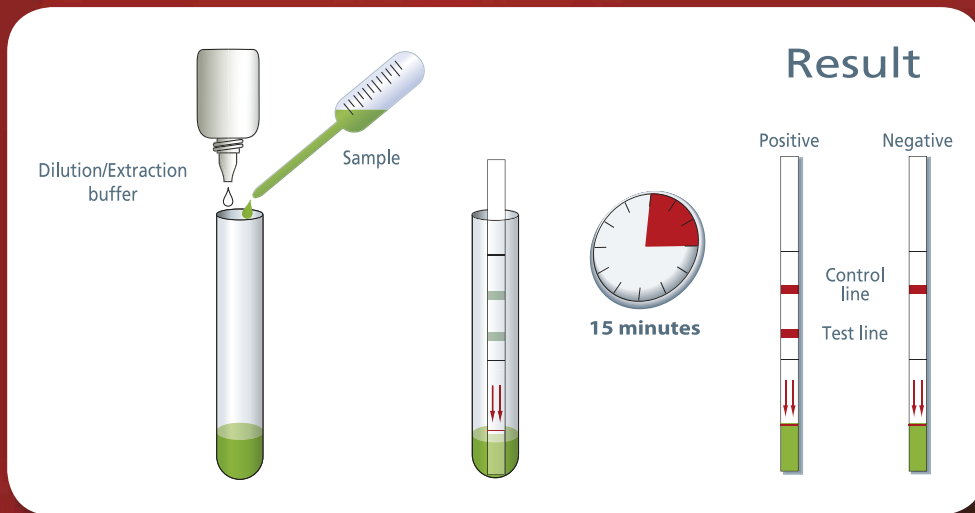

Performance compared to

	RT-PCR (n=113)	TR-FIA (n=89)
Specificity	100% (66/66)	100% (56/56)
Sensitivity	76.6% (36/47)	97% (32/33)
PPV	100% (36/36)	100% (32/32)
NPV	85.7% (66/77)	98.2% (56/57)
Accuracy	90.3% (102/113)	98.9% (88/89)

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
Influ-A Respi-Strip	25 tests, buffer	4°C to 30°C	C-1010
Influ-A Respi K-SeT	20 cassettes, buffer	4°C to 30°C	K-1210
Influ-A Respi K-SeT, with collection set	20 cassettes, buffer, 20 swabs	4°C to 30°C	K-1510

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, Mefloquine, Proguanil, *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

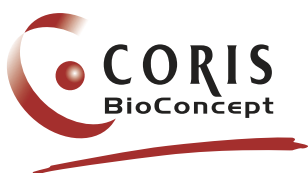

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-10/04
January 2012