

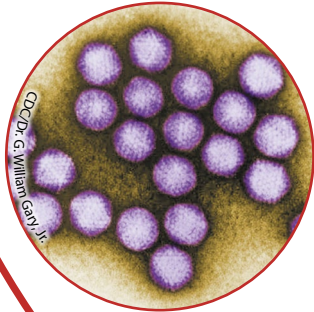


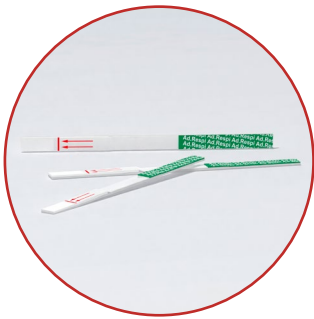

Adeno Respi-Strip


Rapid diagnostic test for *in vitro* detection of Respiratory Adenovirus in nasopharyngeal secretions

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')

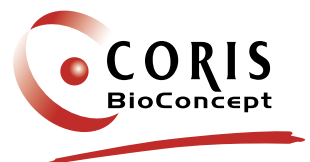

www.corisbio.com

Adeno Respi-Strip

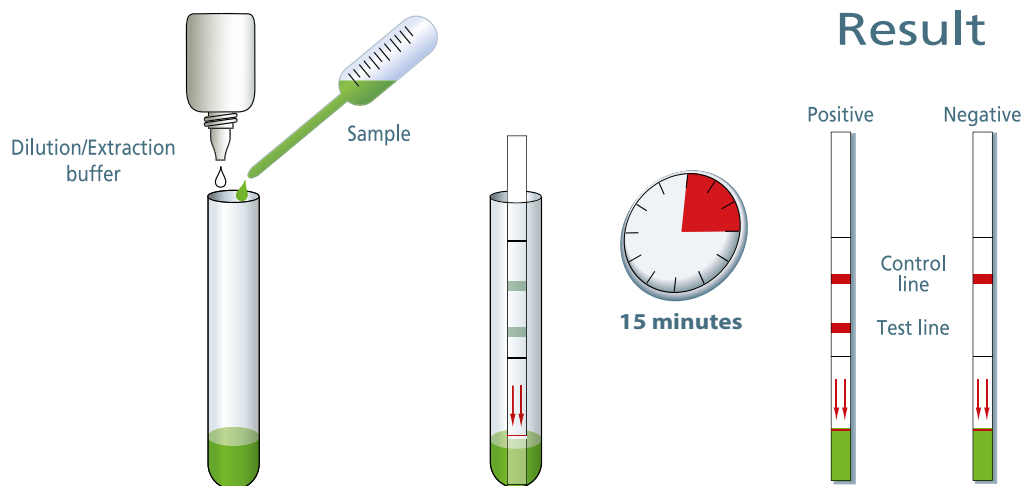

Performance of the kit


	Compared to ICT competitor 1 (n=127)		Compared to ICT competitor 2 (n=127)	
		(95% confidence interval)		(95% confidence interval)
Sensitivity	92.3 %	(80.6 to 97.5 %)	94 %	(82.5 to 98.4 %)
Specificity	96 %	(88 to 99 %)	94.8 %	(86.5 to 98.3 %)
PPV	94.1 %	(82.8 to 98.5 %)	92.2 %	(80.3 to 97.5 %)
NPV	94.7 %	(86.4 to 98.3 %)	96.1 %	(88.1 to 99 %)
Agreement	94.5 %	(120/127)	94.5 %	(120/127)

For more technical information

client.care@corisbio.com


Ordering Information

PRODUCT NAME	DESCRIPTION	STORAGE	CODE
Adeno Respi-Strip	25 tests, buffer	4°C to 30°C	C-1009
Adeno Respi K-SeT	20 cassettes, buffer	4°C to 30°C	K-1209
Adeno Respi K-SeT with collection set	20 cassettes, buffers, 20 swabs, 20 tube-droppers	4°C to 30°C	K-1509



CREALYS Science Park
Rue Guillaume Fouquet 11
5032 Gembloux - BELGIUM
T +32 (0)81 719 910 - F +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

— Distributed by —



D-CUS-10-09-S/10
March 2023

MADE IN BELGIUM