

Combi-Strip


Rapid diagnostic test for *in vitro* detection of
Rotavirus & Adenovirus in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')



www.corisbio.com

Combi-Strip

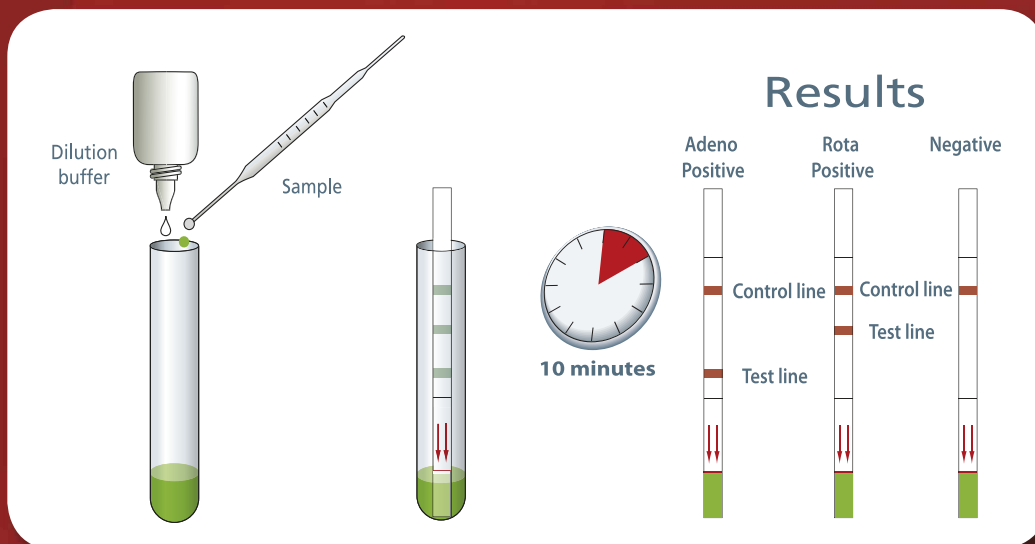

Performance compared to EIA

| | Rotavirus detection (n=214) | Adenovirus detection (n=130) |
|-------------|-----------------------------|------------------------------|
| Specificity | 100% (108/108) | 100% (118/118) |
| Sensitivity | 99.1% (105/106) | 100% (12/12) |
| PPV | 100% (105/105) | 100% (12/12) |
| NPV | 99.1% (108/109) | 100% (118/118) |
| Accuracy | 99.5% (213/214) | 100% (130/130) |

For more technical information

client.care@corisbio.com


Ordering Information

| Product Name | Description | Storage | Code |
|-------------------------------------|---|-------------|--------|
| Combi-Strip | 25 tests, buffer | 4°C to 30°C | C-1004 |
| Combi K-SeT | 20 cassettes, buffer | 4°C to 30°C | K-1204 |
| Combi K-SeT, with collection set | 20 cassettes, buffer, 20 faecal sampling systems | 4°C to 30°C | K-1504 |

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus. Mefloquine, Proguanil. *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

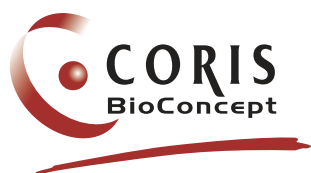

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-04/06
January 2012