

GastroVir K-Set


Rapid diagnostic test for *in vitro* detection of Rotavirus & group F Adenovirus in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')
- Multiple coloured lines



www.corisbio.com

GastroVir K-SeT

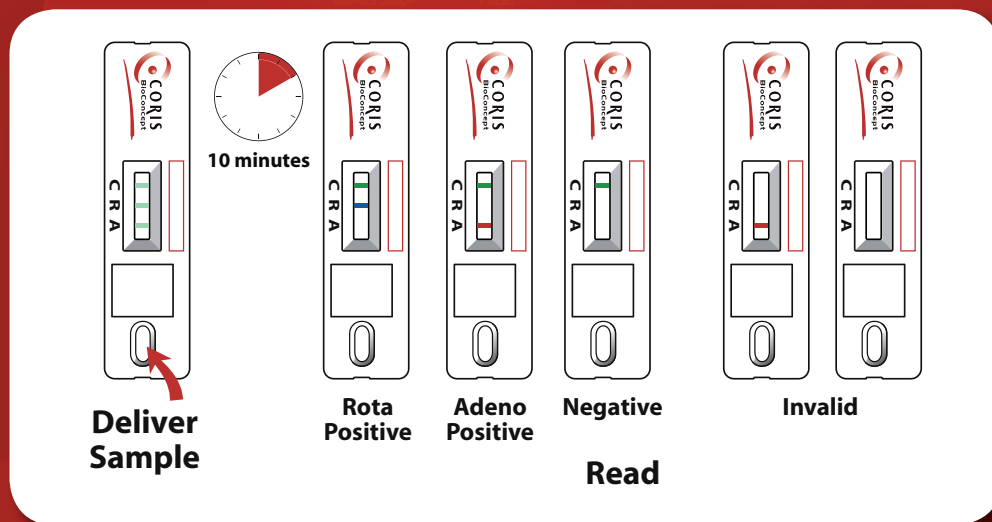

Performances of the test:

	Rotavirus detection Compared to PAGE method (n=400) (95% confidence interval)	Adenovirus 40 and 41 detection Compared to PCR method (n=400) (95% confidence interval)
Specificity	97.9% (95.2 to 99.1%)	97.3% (94.9 to 98.6%)
Sensitivity	97.4% (92.1 to 99.3%)	96.7% (80.1 to 99.8%)
PPV	95.0% (88.9 to 97.9%)	74.4% (57.6 to 86.4%)
NPV	98.9% (96.7 to 99.7%)	99.7% (98.2 to 100%)
Accuracy	97.8%	97.3%

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
GastroVir K-SeT	20 tests, buffer	4°C to 30°C	K-1216
GastroVir K-SeT, with collection set	20 tests, buffer, 20 faecal sampling systems	4°C to 30°C	K-1516
GastroVir-Strip	25 tests, buffer	4°C to 30°C	C-1016

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, *Giardia*, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, *Trypanosoma brucei gambiense*.
Mefloquine, Proguanil.
Leishmania spp., *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

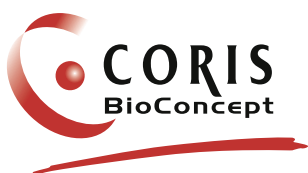

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-16/04
August 2014