



Pylori-Strip


Rapid diagnostic test for *in vitro* detection of *Helicobacter pylori* antigen in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')
- Multiple coloured lines



www.corisbio.com

Pylori-Strip

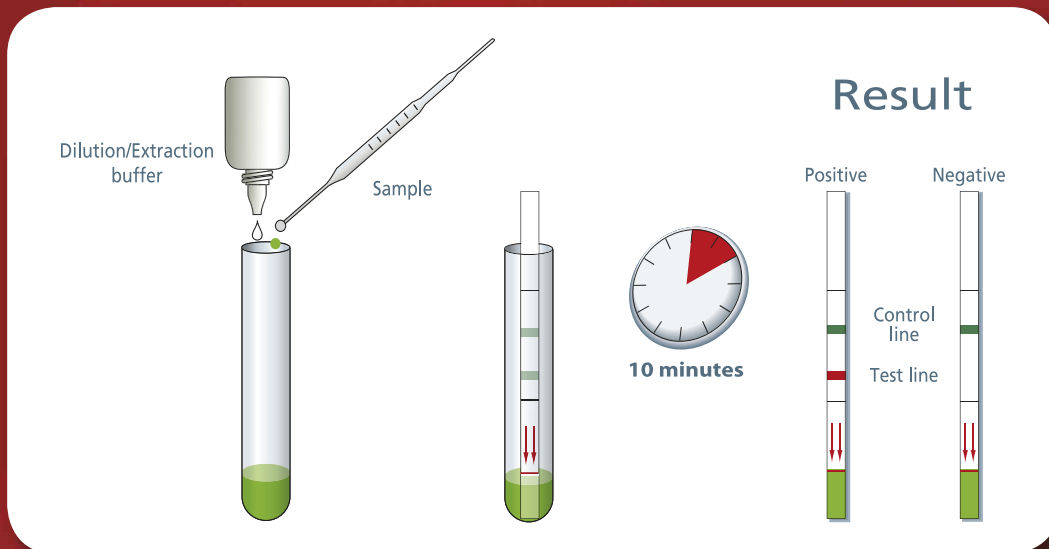

Performance compared to EIA (n = 93)

Specificity	97.1% (33/34)
Sensitivity	96.6% (57/59)
PPV	98.3% (57/58)
NPV	94.3% (33/35)
Accuracy	96.8% (90/93)

For more technical information

client.care@corisbio.com


Ordering Information

Product Name	Description	Storage	Code
Pylori-Strip	25 tests, buffer	4°C to 30°C	C-1019
Pylori K-SeT	20 cassettes, buffer	4°C to 30°C	K-1219
Pylori K-SeT	20 cassettes, 20 faecal sampling systems	4°C to 30°C	K-1519

All diagnostics available in Coris BioConcept catalogue :

Adenovirus, Adenovirus (Respiratory), Adenovirus 40 and 41, *Clostridium difficile*, Bovine Coronavirus, *Cryptosporidium*, *Escherichia coli* O157, *Escherichia coli* K99, Giardia, *Helicobacter pylori*, Influenza A and B viruses, *Legionella pneumophila*, Respiratory Syncytial Virus, Rotavirus, Mefloquine, Proguanil, *Leishmania spp.*, *Trypanosoma cruzi*, *P. aeruginosa* efflux.

Distributed by:

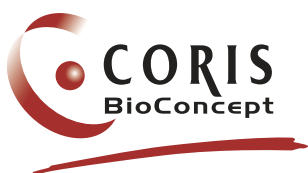

Science Park CREALYS
 Rue Jean Sonet 4A - 5032 Gembloux - Belgium
 Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

Fo 7.5-32-19/03
 January 2012