


Clostridium K-Set


Rapid diagnostic test for *in vitro* detection of *Clostridium difficile* antigen in stool specimens

- Safe
- Easy and ready to use
- Complete set of sampling devices available
- Accurate
- Easy to interpret

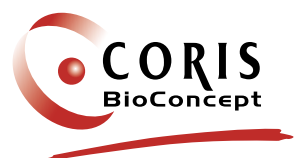

www.corisbio.com

Clostridium K-SeT

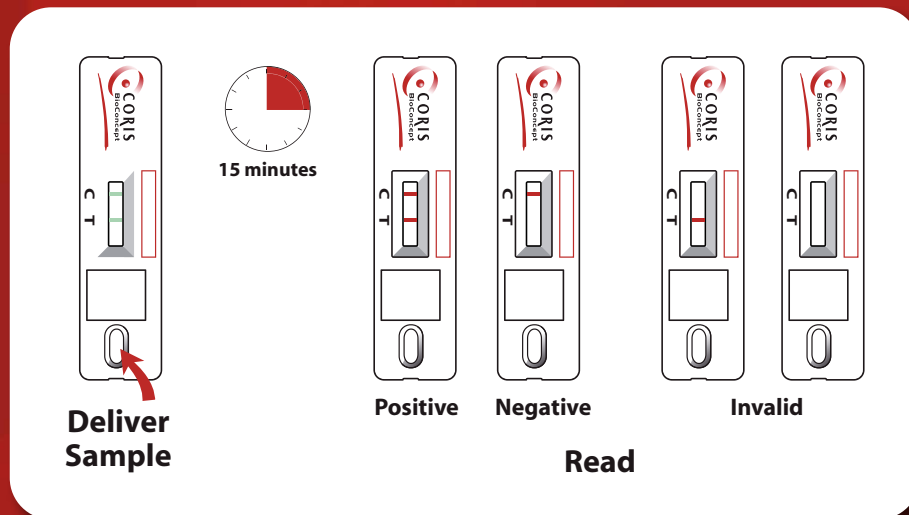

Performance of the test:

Compared to Culture (n=318)

		(95% confidence interval)
Sensitivity	100%	(93.9 to 100%)
Specificity	93%	(88.8 to 95.7%)
PPV	81.5%	(71.8 to 88.6%)
NPV	100%	(97.9 to 100%)
Agreement	94.7%	(301/318)

Compared to ICT (n=318)

		(95% confidence interval)
Sensitivity	100%	(56.1 to 100%)
Specificity	93%	(93.3 to 99.9%)
PPV	87.5%	(46.7 to 99.3%)
NPV	100%	(95 to 100%)
Agreement	99.0%	(99/100)

For more technical information

client.care@corisbio.com

Ordering Information

Product name	Description	Storage	Code
Clostridium K-SeT	20 cassettes, buffer	4°C to 30°C	K-1220
Clostridium K-SeT	20 cassettes, 20 faecal sampling systems	4°C to 30°C	K-1520
C. diff-Strip	25 tests, buffer	4°C to 30°C	C-1020

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

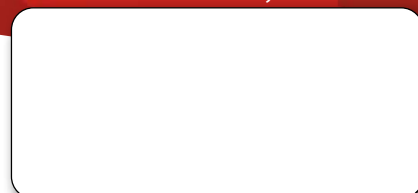

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-20-K/02
February 2020