


Combi K-Set


Rapid diagnostic test for *in vitro* detection of Rotavirus & Adenovirus in stool specimens

- Safe
- Easy and ready to use
- Complete set of sampling devices available
- Accurate
- Easy to interpret

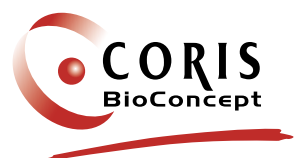

www.corisbio.com

Combi K-SeT

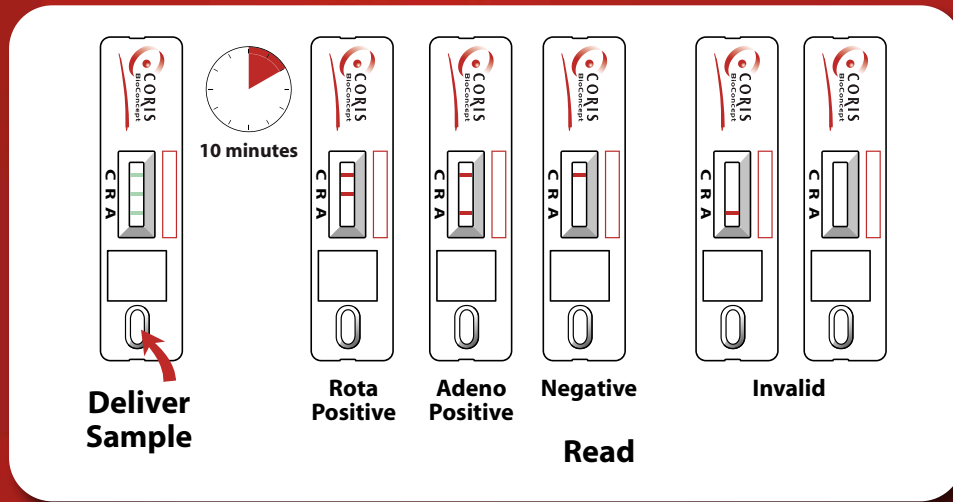

Performance compared to ELISA

	Performance compared to RT-qPCR (n=194)	Performance compared to qPCR (n=190)
	(95% confidence interval)	(95% confidence interval)
Sensitivity	91.7 % (82.1 to 96.6 %)	82.6 % (60.5 to 94.3 %)
Specificity	99.2 % (99.2 to 100 %)	97.0 % (92.8 to 98.9 %)
PPV	98.5 % (90.9 to 99.9 %)	79.2 % (57.3 to 92.1 %)
NPV	95.3 % (89.6 to 98.1 %)	97.6 % (93.6 to 99.2 %)
Agreement	96.4 % (187/194)	95.3 % (181/190)

For more technical information

client.care@corisbio.com

Ordering Information

Product Name	Description	Storage	Code
Combi K-SeT	20 cassettes, buffer	4°C to 30°C	K-1204
Combi K-SeT, with collection set	20 cassettes, buffer, 20 faecal sampling systems	4°C to 30°C	K-1504
Combi-Strip	20 tests, buffer	4°C to 30°C	C-1004

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

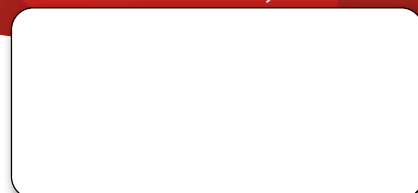

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-04-K/02
February 2020