

Crypto/Giardia Duo-Strip


Rapid diagnostic test for *in vitro* detection of *Cryptosporidium* & *Giardia* in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')
- One-side stick



www.corisbio.com

Crypto/Giardia Duo-Strip

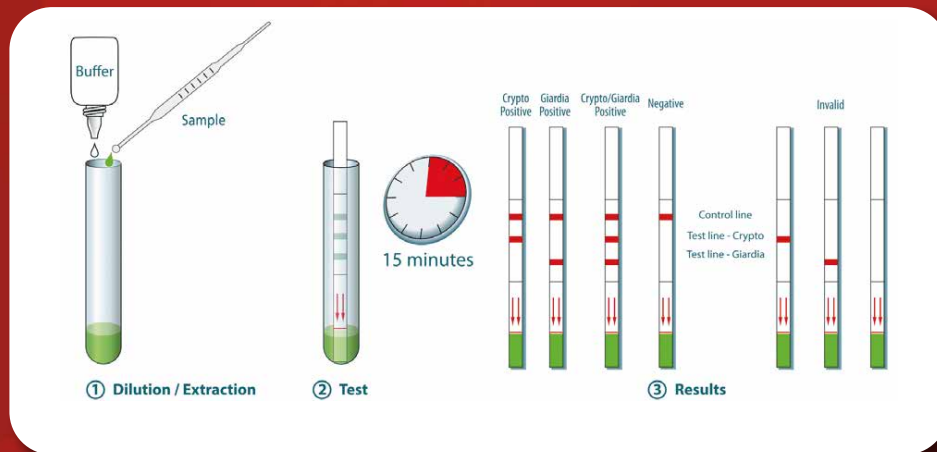

Performance compared to Microscopic analysis

	Cryptosporidium (n=184) (95% confidence interval)	Giardia (n=184) (95% confidence interval)
Sensitivity	86.7% (68.4 to 95.6%)	89.2% (73.6 to 96.5%)
Specificity	100% (97.0 to 100%)	99.3% (95.7 to 100%)
PPV	100% (84.0 to 100%)	97.1% (83.0 to 99.9%)
NPV	97.5% (93.2 to 99.2%)	97.3% (92.9 to 99.1%)
Agreement	97.8% (180/184)	97.3% (179/184)

For more technical information

client.care@corisbio.com

Ordering Information

Product Name	Description	Storage	Code
Crypto/Giardia Duo-Strip	25 tests, buffer	4°C to 30°C	C-1018

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

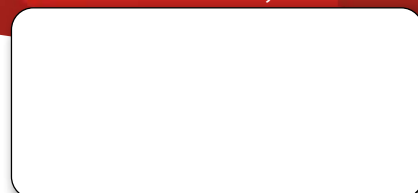

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-18-S/04
February 2020