




Giardia-Strip


Rapid diagnostic test for *in vitro* detection of *Giardia* in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')



www.corisbio.com

Giardia-Strip

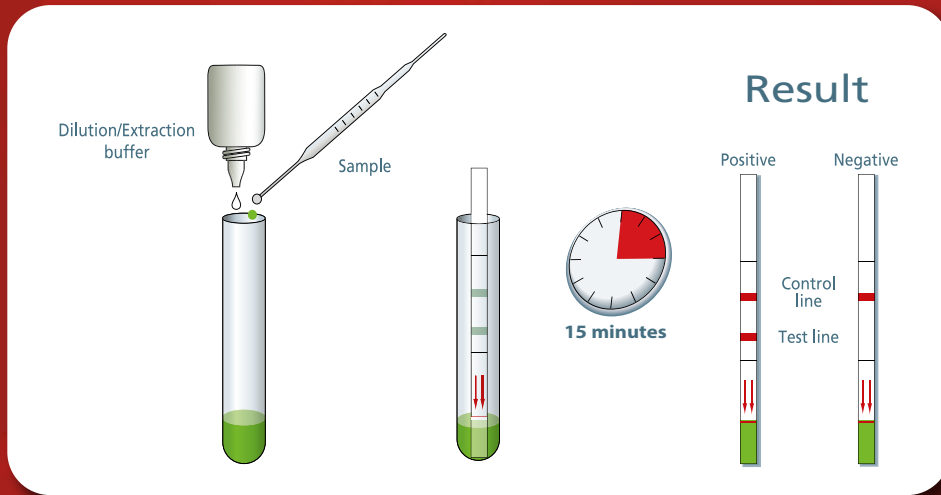

Performance compared to

	ELISA (n=94) (95% confidence interval)	Microscopic analysis (n=56) (95% confidence interval)
Sensitivity	100 % (81.5 to 100 %)	100 % (71.7 to 100 %)
Specificity	95.8 % (87.5 to 98.9 %)	95.3 % (82.9 to 92.2 %)
PPV	88.0 % (67.7 to 96.9 %)	86.7 % (58.4 to 97.7 %)
NPV	100 % (93.4 to 100 %)	100 % (89.3 to 100 %)
Agreement	96.8 % (91/94)	96.4 % (54/56)

For more technical information

client.care@corisbio.com

Ordering Information

Product Name	Description	Storage	Code
Giardia-Strip	25 tests, buffer	4°C to 30°C	C-1013
Giardia K-SeT	20 cassettes, buffer	4°C to 30°C	K-1213
Giardia K-SeT, with collection set	20 cassettes, 20 faecal sampling systems	4°C to 30°C	K-1513

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

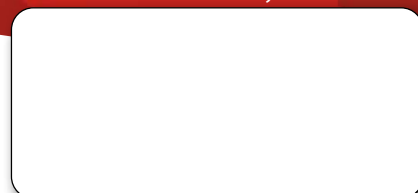

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-13-S/15
February 2020