




Pylori K-Set


Rapid diagnostic test for *in vitro* detection of *Helicobacter pylori* antigen in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')
- Multiple coloured lines

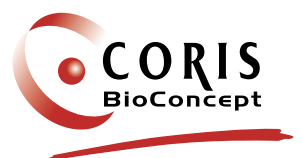

www.corisbio.com

Pylori K-SeT

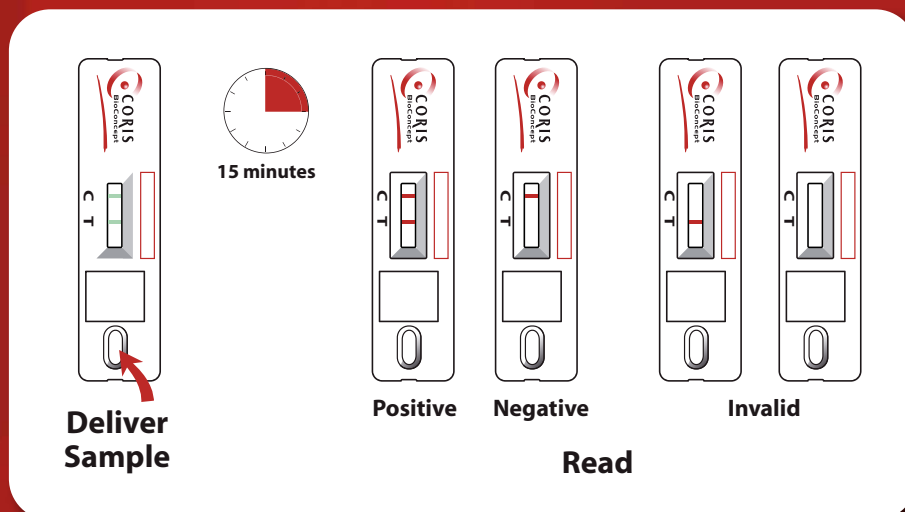

Performance compared to EIA (n = 134)

		(95% confidence interval)
Sensitivity	96.0%	(77.7 to 99.8%)
Specificity	98.2%	(92.9 to 99.7%)
PPV	92.3%	(73.4 to 98.7%)
NPV	99.1%	(94.2 to 100%)
Agreement	97.8%	(131/134)

For more technical information

client.care@corisbio.com

Ordering Information

Product Name	Description	Storage	Code
Pylori K-SeT	20 cassettes, buffer	4°C to 30°C	K-1219
Pylori K-SeT	20 cassettes, 20 faecal sampling systems	4°C to 30°C	K-1519
Pylori-Strip	25 tests, buffer	4°C to 30°C	C-1019

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

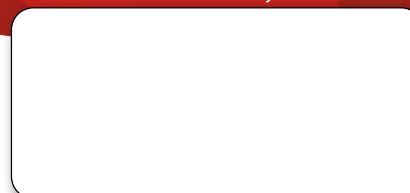

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-19-K/02
February 2020