




Pylori-Strip


Rapid diagnostic test for *in vitro* detection of *Helicobacter pylori* antigen in stool specimens

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (10')
- Multiple coloured lines

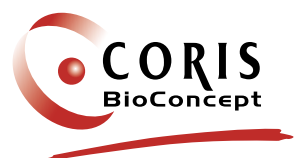

www.corisbio.com

Pylori-Strip

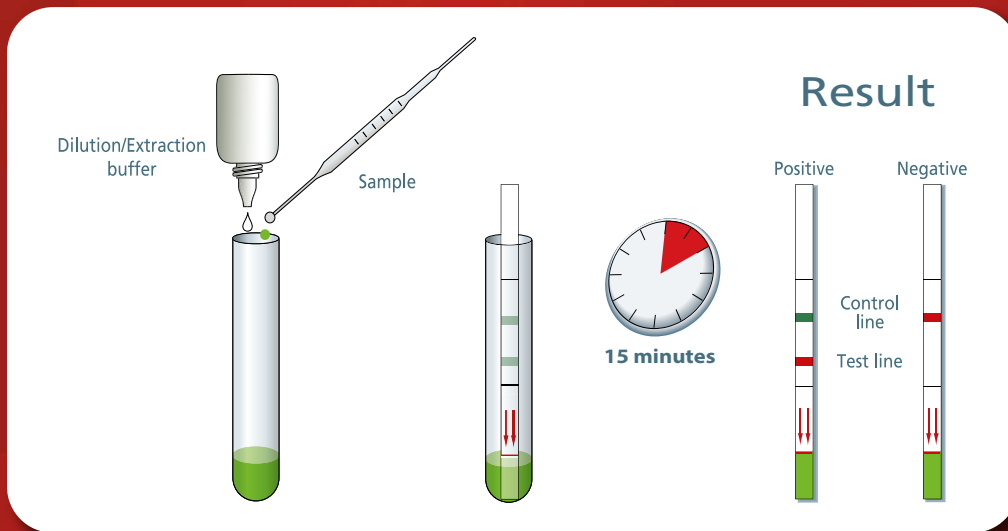

Performance compared to EIA (n = 134)

| | | (95% confidence interval) |
|-------------|-------|---------------------------|
| Sensitivity | 96.0% | (77.7 to 99.8%) |
| Specificity | 98.2% | (92.9 to 99.7%) |
| PPV | 92.3% | (73.4 to 98.7%) |
| NPV | 99.1% | (94.2 to 100%) |
| Agreement | 97.8% | (131/134) |

For more technical information

client.care@corisbio.com

Ordering Information

| Product Name | Description | Storage | Code |
|--------------|--|-------------|--------|
| Pylori-Strip | 25 tests, buffer | 4°C to 30°C | C-1019 |
| Pylori K-SeT | 20 cassettes, buffer | 4°C to 30°C | K-1219 |
| Pylori K-SeT | 20 cassettes, 20 faecal sampling systems | 4°C to 30°C | K-1519 |

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

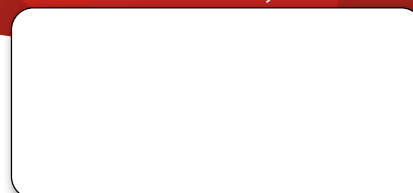

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-19-S/04
February 2020