


RSV K-Set


Rapid diagnostic test for *in vitro* detection of Respiratory Syncytial Virus in nasopharyngeal specimens

- Safe
- Easy and ready to use
- Complete set of sampling devices available
- Accurate
- Easy to interpret

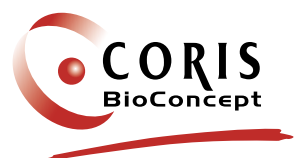

www.corisbio.com

RSV K-SeT

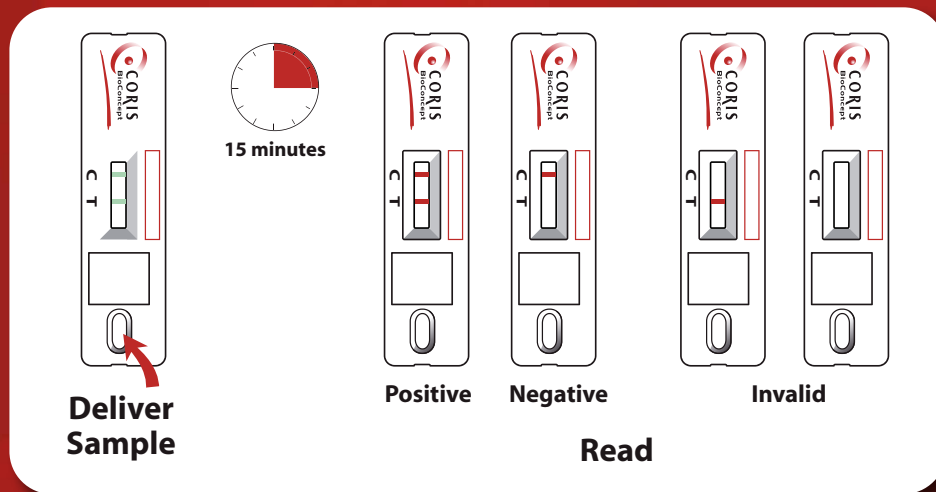

Performance compared to

| | IF (n=100) | | DFA (n=236) | |
|-------------|------------|---------------------------|-------------|---------------------------|
| | | (95% confidence interval) | | (95% confidence interval) |
| Sensitivity | 96% | (85.1 to 99.3%) | 92.2 % | (85.2 to 96.1%) |
| Specificity | 100% | (91.1 to 100%) | 98.3 % | (93.6 to 99.7%) |
| PPV | 100% | (90.8 to 100%) | 98.1 % | (92.8 to 99.7%) |
| NPV | 96.2% | (85.7 to 99.3%) | 93% | (92.9 to 96.5%) |
| Agreement | 98% | (98/100) | 95.3% | (225/236) |

For more technical information

client.care@corisbio.com

Ordering Information

| Product Name | Description | Storage | Code |
|-----------------------------------|-----------------------------------|-------------|--------|
| RSV K-SeT | 20 cassettes, buffer | 4°C to 30°C | K-1206 |
| RSV K-SeT, with collection set | 20 cassettes, buffer, 20 swabs | 4°C to 30°C | K-1506 |
| RSV Respi-Strip | 25 tests, buffer | 4°C to 30°C | C-1006 |

All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

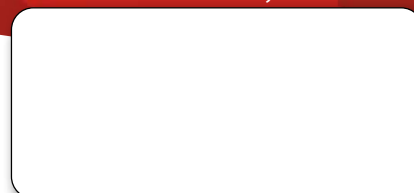

Science Park CREALYS
Rue Jean Sonet 4A - 5032 Gembloux - Belgium
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-06-K/03
February 2020