


# RSV Respi-Strip


**Rapid diagnostic test for *in vitro* detection of Respiratory Syncytial Virus in nasopharyngeal specimens**

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')

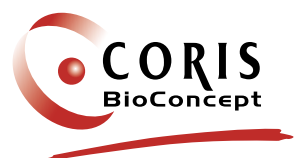

[www.corisbio.com](http://www.corisbio.com)

# RSV Respi-Strip

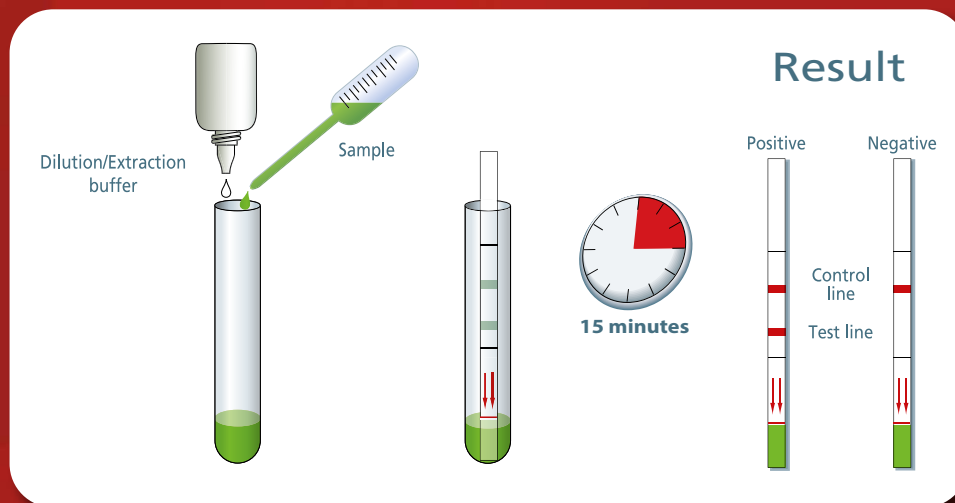

## Performance compared to

	IF (n=100)		DFA (n=236)	
		(95% confidence interval)		(95% confidence interval)
Sensitivity	96%	(85.1 to 99.3%)	92.2 %	(85.2 to 96.1%)
Specificity	100%	(91.1 to 100%)	98.3 %	(93.6 to 99.7%)
PPV	100%	(90.8 to 100%)	98.1 %	(92.8 to 99.7%)
NPV	96.2%	(85.7 to 99.3%)	93%	(92.9 to 96.5%)
Agreement	98%	(98/100)	95.3%	(225/236)

## For more technical information

[client.care@corisbio.com](mailto:client.care@corisbio.com)

## Ordering Information

Product Name	Description	Storage	Code
RSV Respi-Strip	25 tests, buffer	4°C to 30°C	C-1006
RSV K-SeT	20 cassettes, buffer	4°C to 30°C	K-1206
RSV K-SeT, with collection set	20 cassettes, buffer, 20 swabs	4°C to 30°C	K-1506

### All diagnostics available in Coris BioConcept catalogue:

Virus: 40/41 Adenovirus, Adenovirus, Influenza A&B, Respiratory Adenovirus, Respiratory Syncytial Virus, Rotavirus



Bacteria: *Clostridium difficile*, *Helicobacter pylori*, *Legionella pneumophila*, *Streptococcus* (group A)

Parasite: *Cryptosporidium*, *Giardia*, *Human African Trypanosomiasis*

Antimicrobial Resistance (RESIST): OXA-23, OXA-48, OXA-163, IMP, KPC, NDM, VIM

Drug monitoring: Mefloquine, Proguanil

Distributed by:

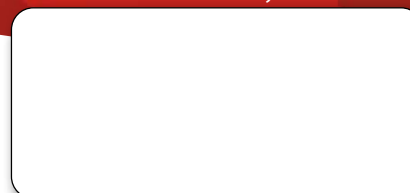

Science Park CREALYS  
Rue Jean Sonet 4A - 5032 Gembloux - Belgium  
Ph.: +32 (0) 81 719 910 - Fx.: +32 (0)81 719 919  
sales@corisbio.com - www.corisbio.com

MADE IN BELGIUM

D-CUS-10-06-5/09  
February 2020