


# RSV Respi-Strip


**Rapid diagnostic test for *in vitro* detection of Respiratory Syncytial Virus in nasopharyngeal secretions**

- Easy to use
- Easy to read
- Specific
- Sensitive
- Reliable
- Rapid (15')

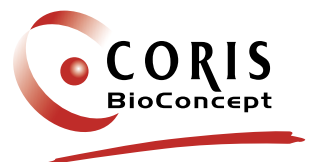

[www.corisbio.com](http://www.corisbio.com)

# RSV Respi-Strip

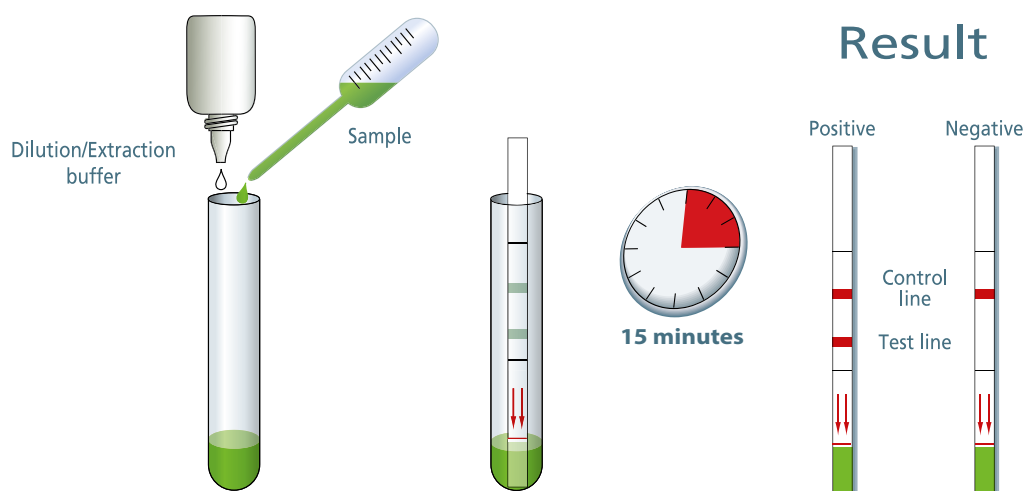

## Performance of the kit

	Compared to Culture (n=500) (95% confidence interval)		Compared to DFA (n=236) (95% confidence interval)	
Sensitivity	90%	(84.2 to 93.9%)	92.2 %	(85.2 to 96.1%)
Specificity	93.3%	(89.9 to 95.7%)	98.3 %	(93.6 to 99.7%)
PPV	87.4%	(81.4 to 91.8%)	98.1 %	(92.8 to 99.7%)
NPV	94.8%	(91.6 to 96.8%)	93%	(92.9 to 96.5%)
Agreement	92.2%	(461/500)	95.3%	(225/236)


## For more technical information

[client.care@corisbio.com](mailto:client.care@corisbio.com)

## Ordering Information

PRODUCT NAME	DESCRIPTION	STORAGE	CODE
RSV Respi-Strip	25 tests, buffer	4°C to 30°C	C-1006
RSV K-SeT	20 cassettes, buffer	4°C to 30°C	K-1206
RSV K-SeT with collection set	20 cassettes, buffer, 20 swabs, 20 tube-droppers	4°C to 30°C	K-1506

— Distributed by —



CREALYS Science Park  
Rue Guillaume Fouquet 11  
5032 Gembloux - BELGIUM  
T +32 (0)81 719 910 - F +32 (0)81 719 919  
sales@corisbio.com - [www.corisbio.com](http://www.corisbio.com)



D-CUS-10-06-S/11  
March 2023

MADE IN BELGIUM